

FIG. 1

22

Excimer Laser Chamber

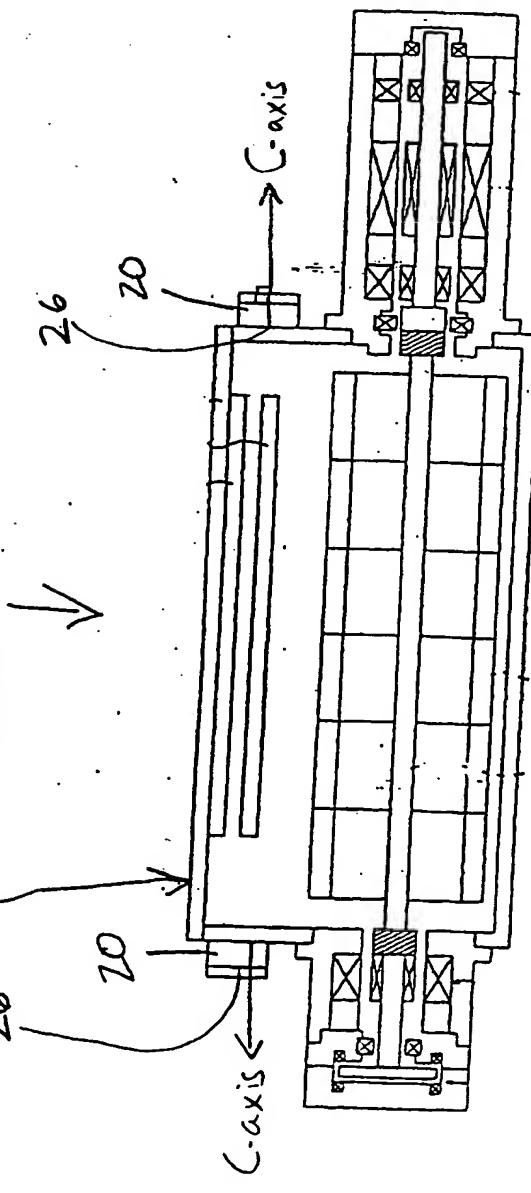


FIG. 2

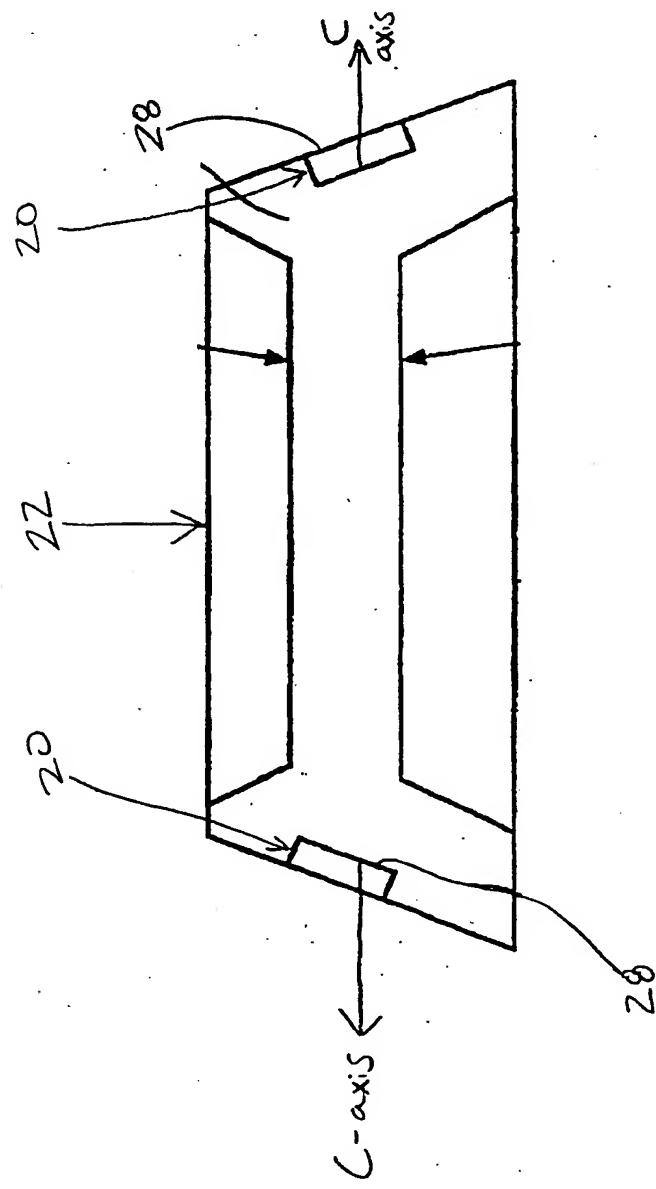


FIG.3

2023-06-07 13:30:20 CT
MgF₂ Sample A
Unexposed vs Exp 4.5E6 @ 193nm
F(avg):40mJ/cm², Path: 42mm

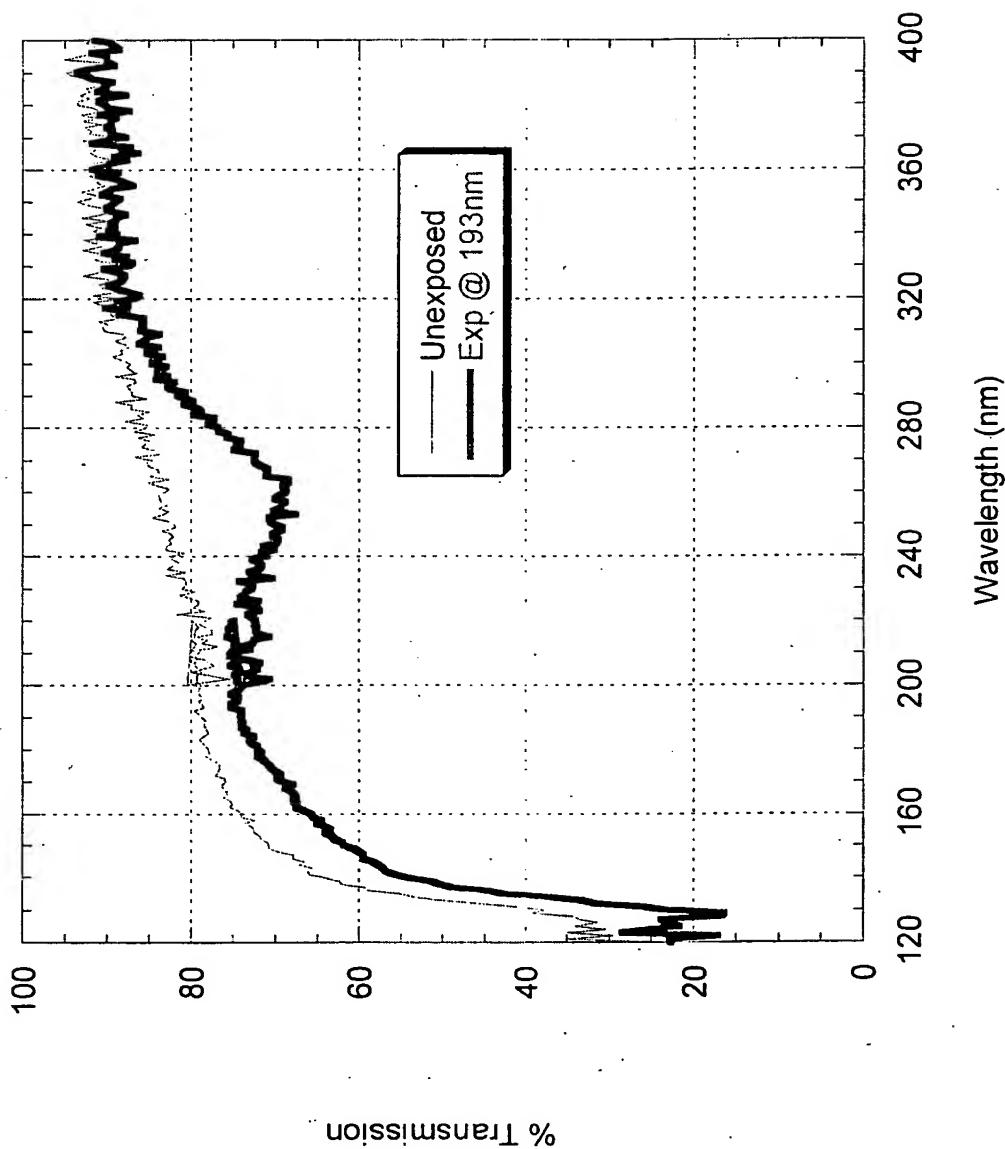


FIG. 4

MgF₂ Sample B
Unexposed vs Exp 4.6E6 @ 193nm
F(avg):40mj/cm², Path: 42mm

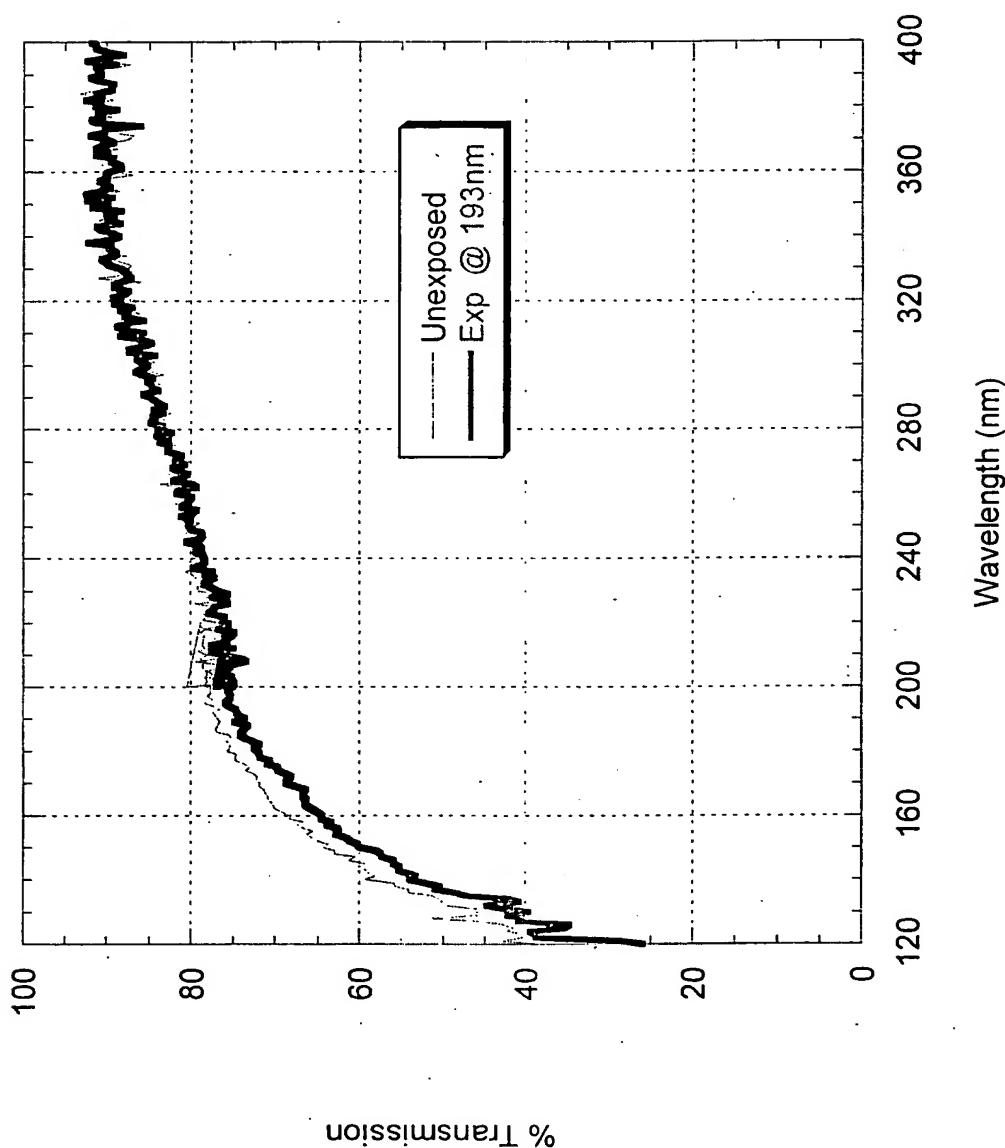


FIG. 5

2015-05-25 10:55:23

MgF₂ Sample C
Unexposed vs Exp 4.6E6 @ 193nm
F(avg):40mj/cm², Path: 42mm

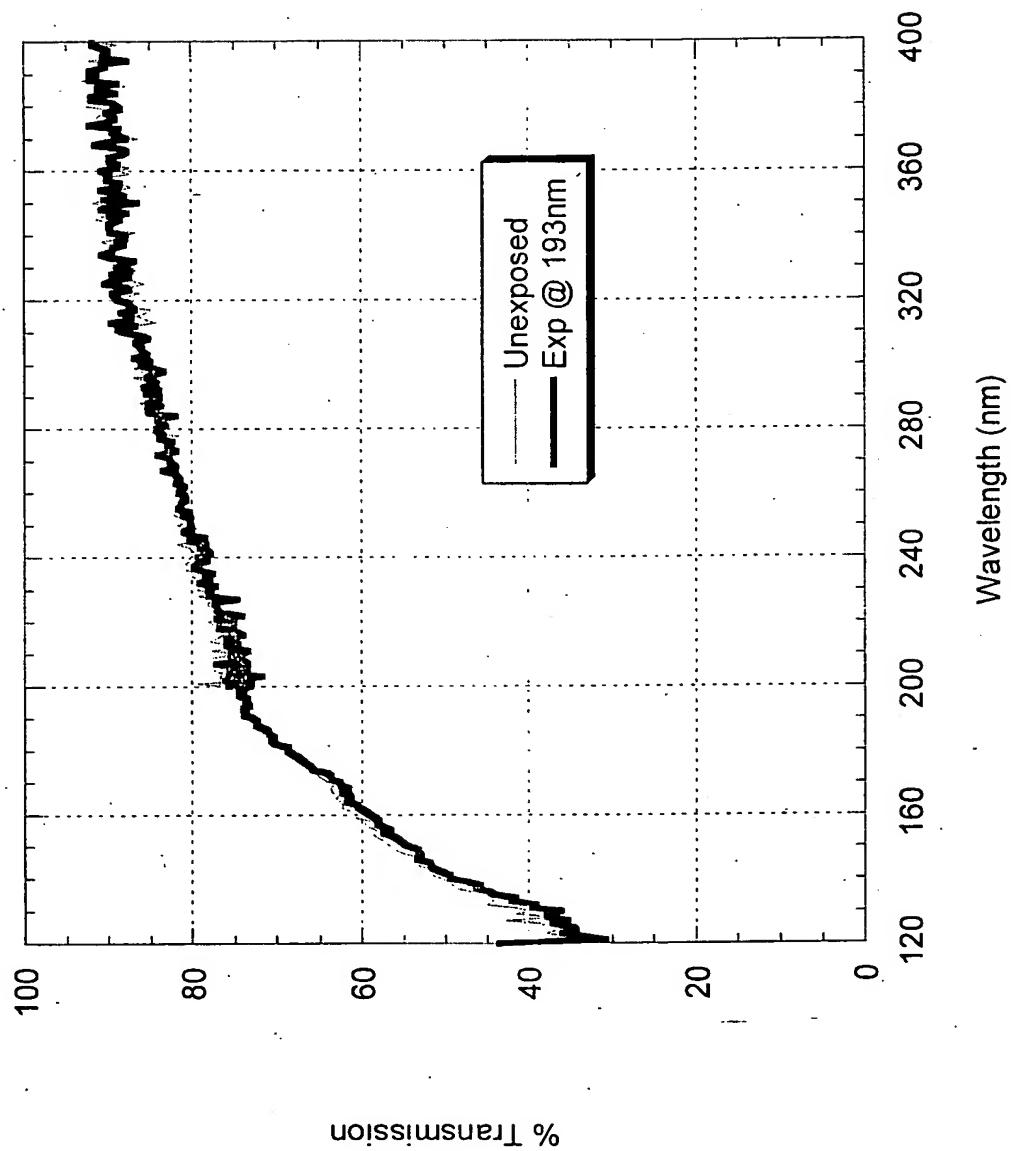


FIG. 6

MgF₂ Sample D
Unexposed vs Exp 4.6E6 @ 193nm
F(avg):40mJ/cm², Path: 42mm

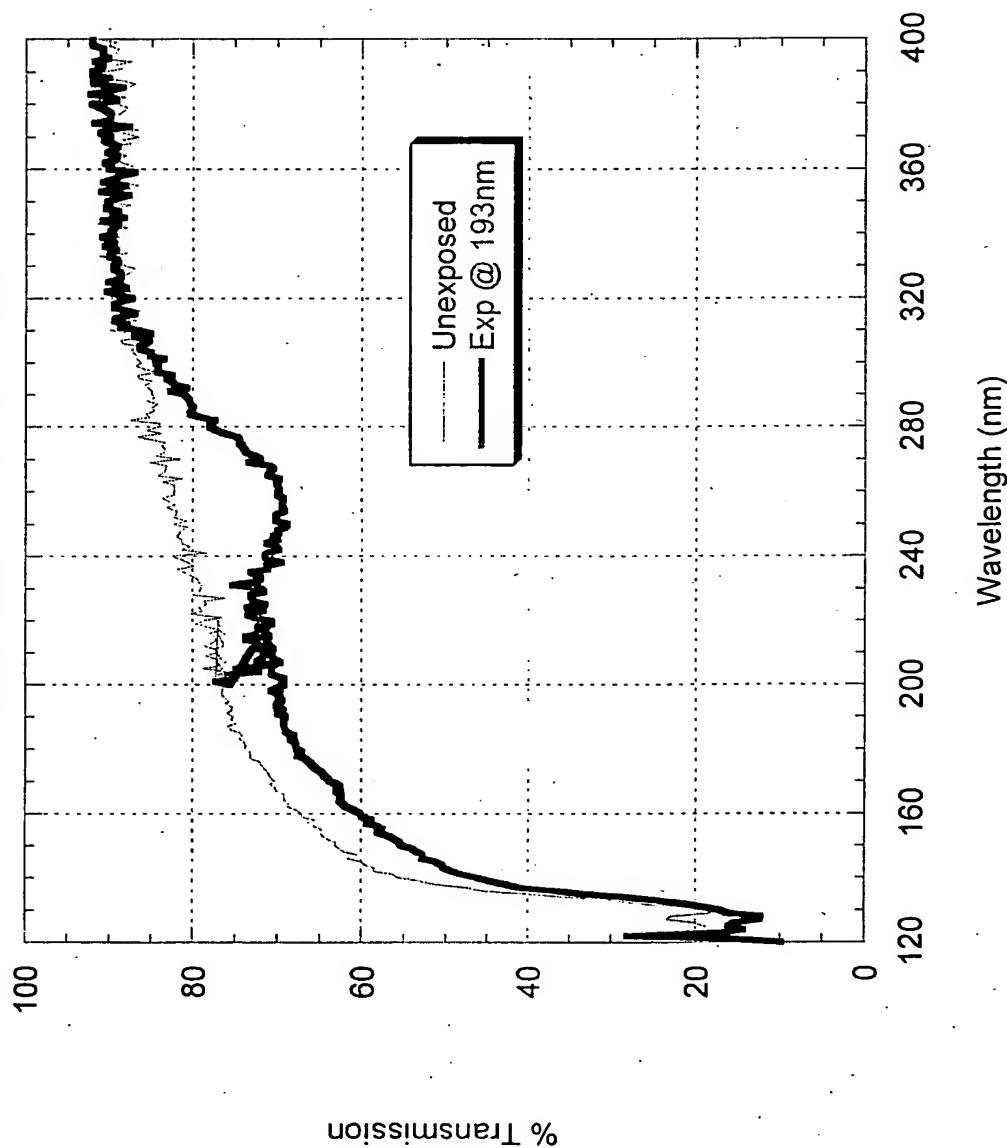


FIG. 7

MgF₂ Sample E
Unexposed vs Exp 4.6E6 @ 193nm
F(avg):40mj/cm², Path: 42mm

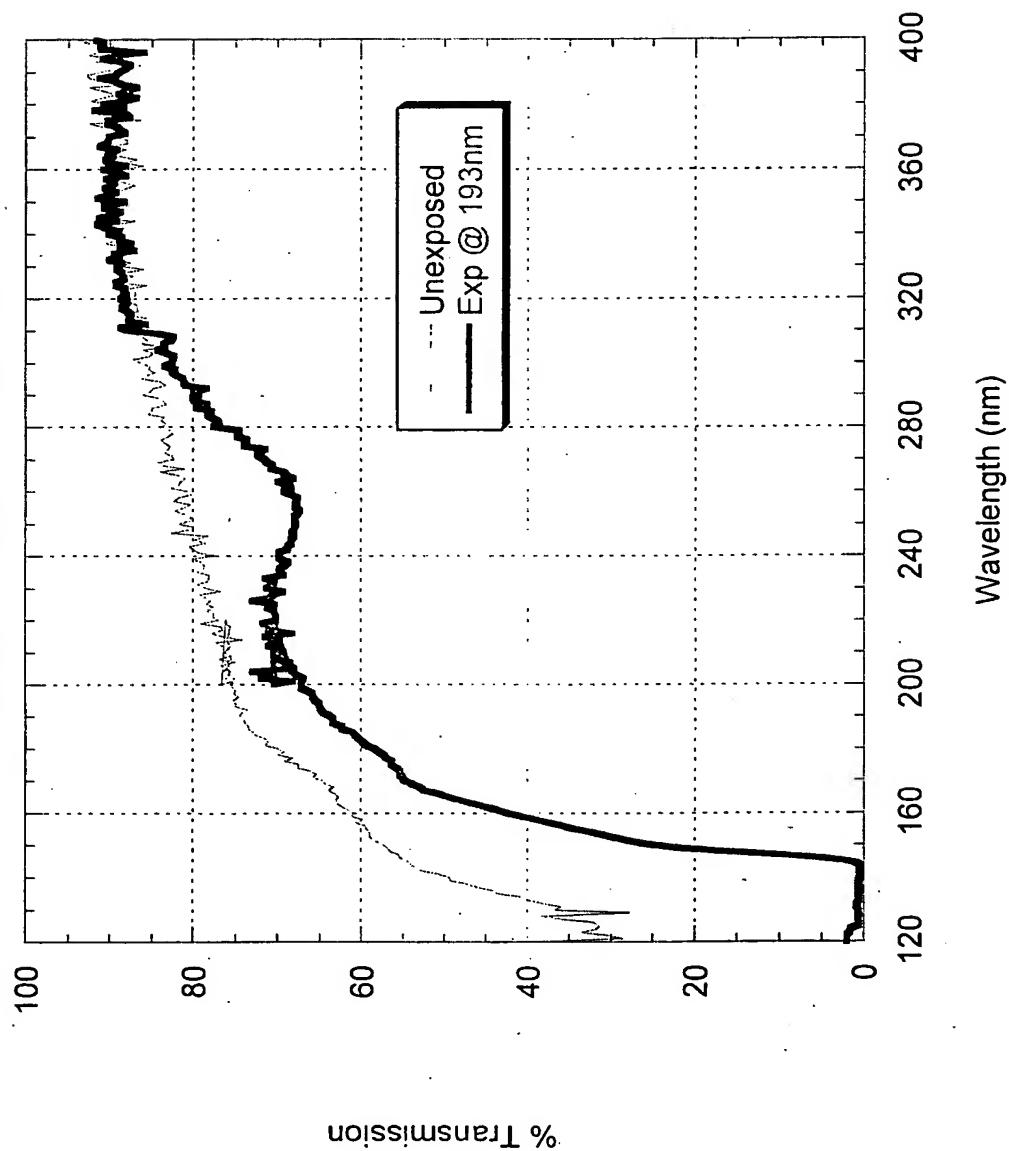


FIG. 8